



## Explorer


## -Single End-



\*Thinness and elasticity at the tip are effective in the check of dental tartar, cavity and surplus cement.



\*A tip part is made thick for intensity.


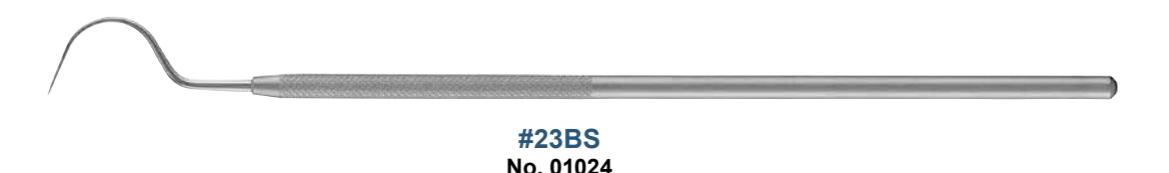


## -Ball Point-



\*The round tip realizes checking of caries without damaging pit and fissure tissues.  
\*Suitable for filling of sealant.

## -Double End-

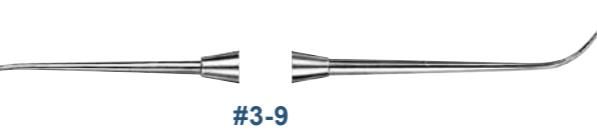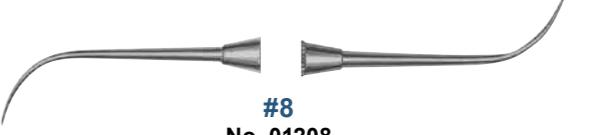

\*Explorer with the shank of "Gracey Curette #11-12".  
\*Thinness and elasticity at the tip are effective in the check of dental tartar, cavity and surplus cement.

## - for Root Canal Therapy -




## Explorer Tip (Replaceable Type)


\*Remove all joint parts and replaceable tip before sterilization and disinfection.  
\*For more replaceable type products see P. 235.

Autoclavable  
up to 135°C  
OK

## -Handle-

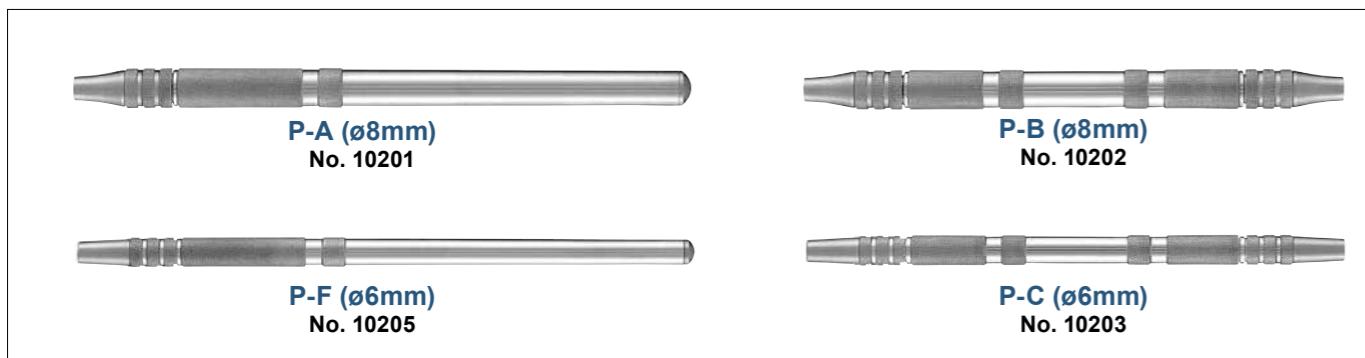


## -Tip (3 ea.)-

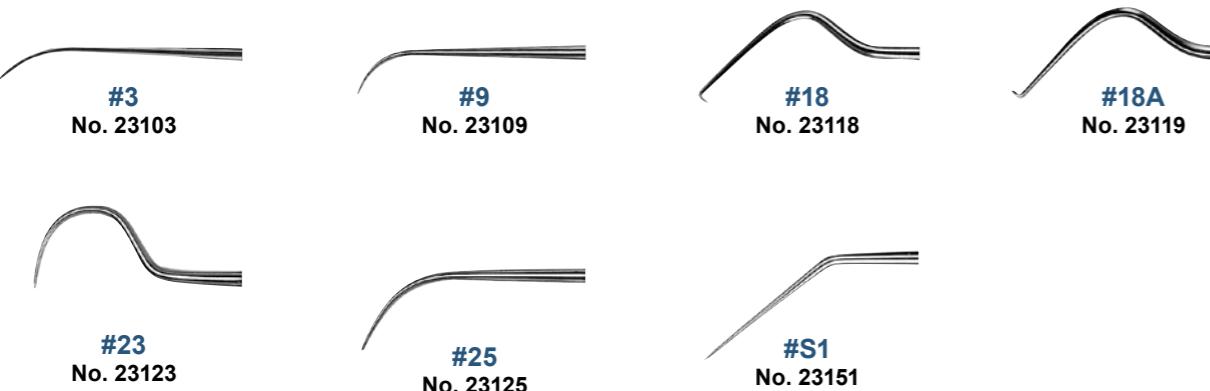

## Excavator

## -Octagonal-

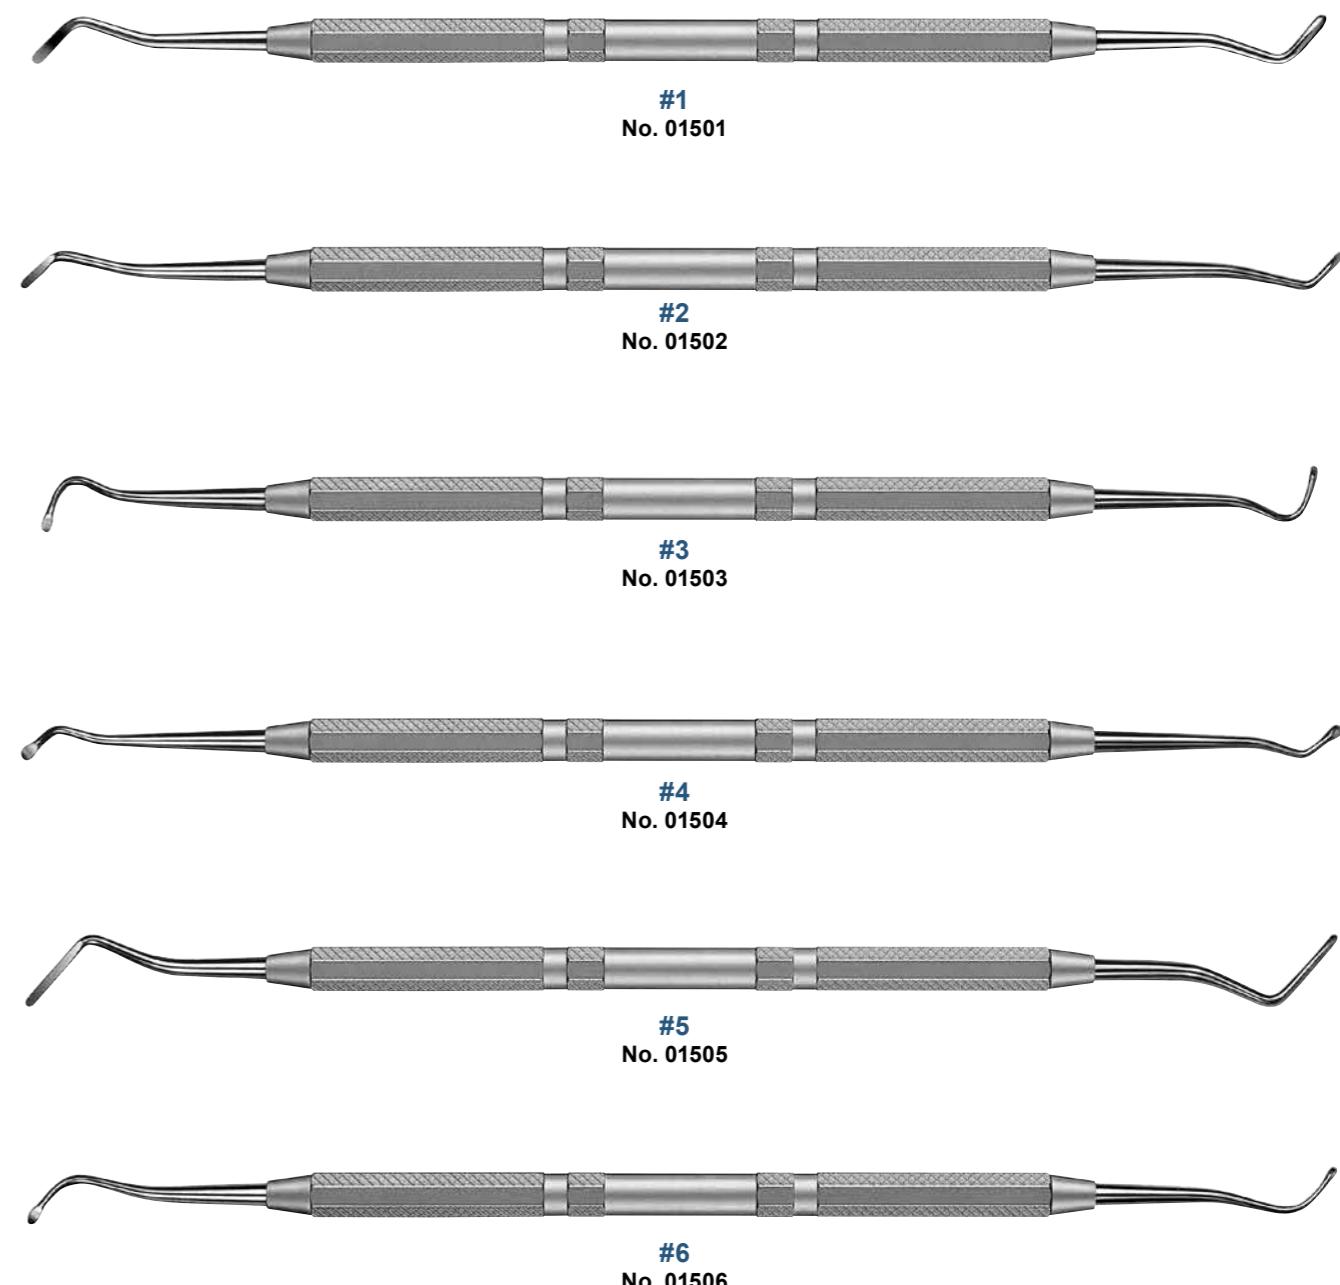

## -Round-

\*Same tips with Octagonal Handle.



#1	#2	#3	#4	#5	#6
01511	01512	01513	01514	01515	01516

Autoclavable  
up to 135°C  
OK

## Dressing Tweezers



**NC #18**  
No. 11305

Size / 160mm



**NC #18 with Serration**  
No. 11306

Size / 160mm



**Mini #18**  
No. 11308

Size / 145mm




**Mini #18 with Serration**  
No. 11309

Size / 145mm



**NC #18 with Diamond**  
No. 11307


Size / 160mm

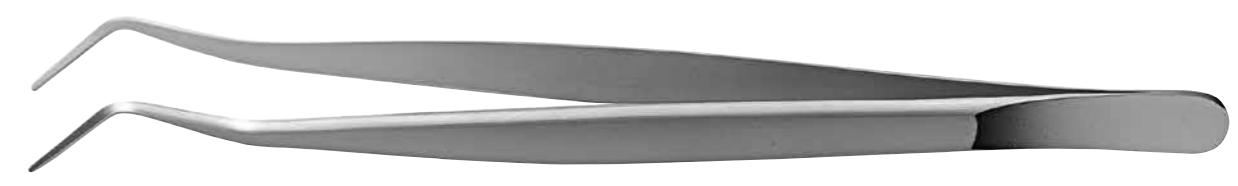

**Premium**  
No. 11019

\*Delicate tweezers.  
\*Careful finish prevents tip misalignment.

Size / 160mm

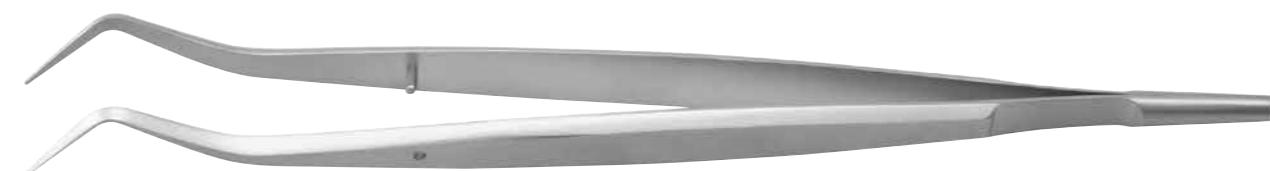

**Koshi**  
No. 11020

Size / 165mm



# Diagnosis

## Mouth Mirror (Simple Stem)

### -Clear 2-

\*With thin glass, there is little blur of an image and reflected vividly.

\*Suitable only for YDM mirror handle.



\*Thickness / 1.9mm



\*Reflection rate / About 93%

### -Front Surface-

#### \*Titanium Coating

\*Direct reflection prevents an image blurring.

\*Suitable only for YDM mirror handle.

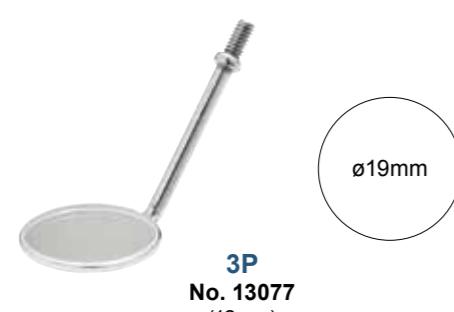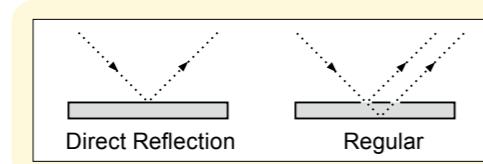


\*Thickness / 1.9mm

\*Reflection rate / About 98%

## Metal Mirror (Simple Stem)

\*The mirror made from stainless steel does not have a fear of being divided, and is suitable for the medical treatment of child dentistry, disabled person dentistry.

\*Suitable only for YDM mirror handle.




\*Thickness / 1.1mm

\*Reflection rate / About 65%



## Mirror Handle

\*Suitable only for YDM mouth mirror.



## Mirror Handle with Millimeter Scale

\*Suitable only for YDM mouth mirror.




\*Material / POM

[How to measure endodontic file or reamer.]



①Fit stopper of reamer or file and pull in the direction of arrow.



②Measure the length of reamer or file with scale on the handle.




③Stopper of reamer or file is fixed.

\*Measurement: Up to 30mm



## Disposable Instrument

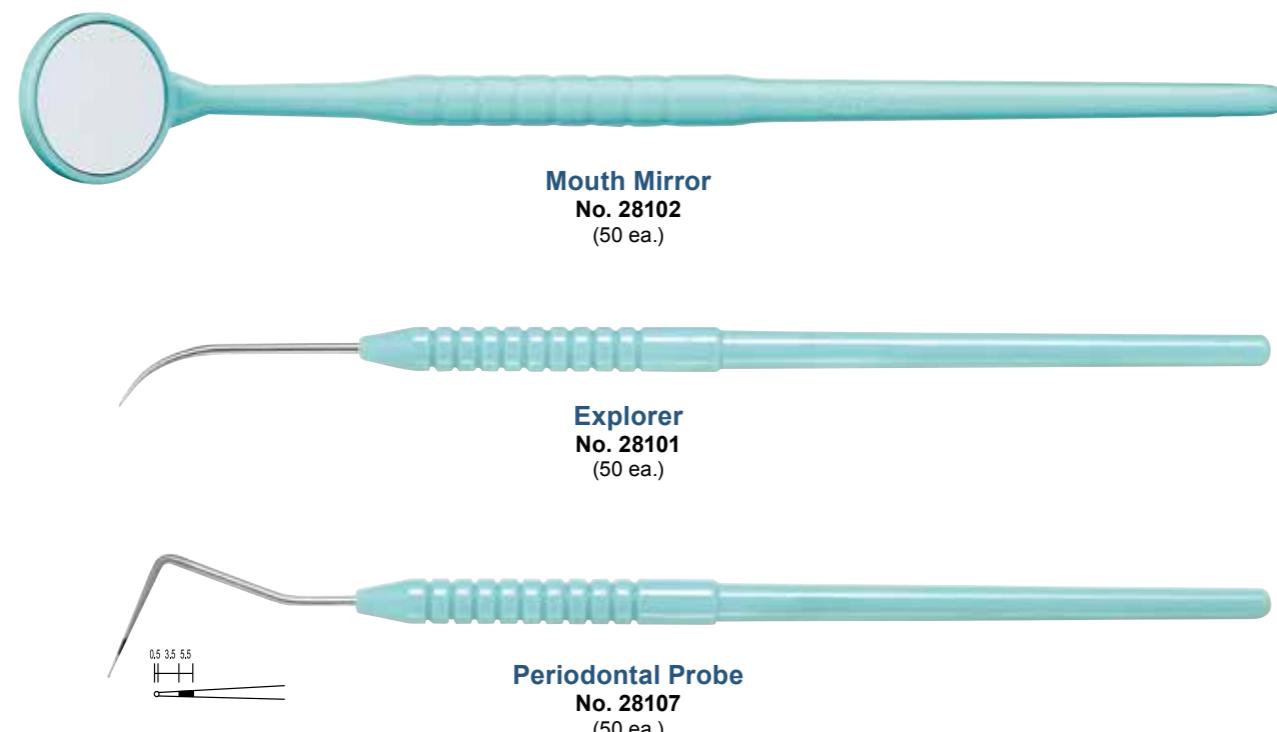


\*Disposable type (Not sterilized)  
\*Material / PS : Heatproof temperature 70°C (Handle)  
\*Need disinfection by solution or EOG sterilization before use.




## Evacuation Tip

## -Universal-

\*There is no trap for suction prevention attached at the evacuation tip, so it is easy to clean. (Rubber sleeve has a trap)

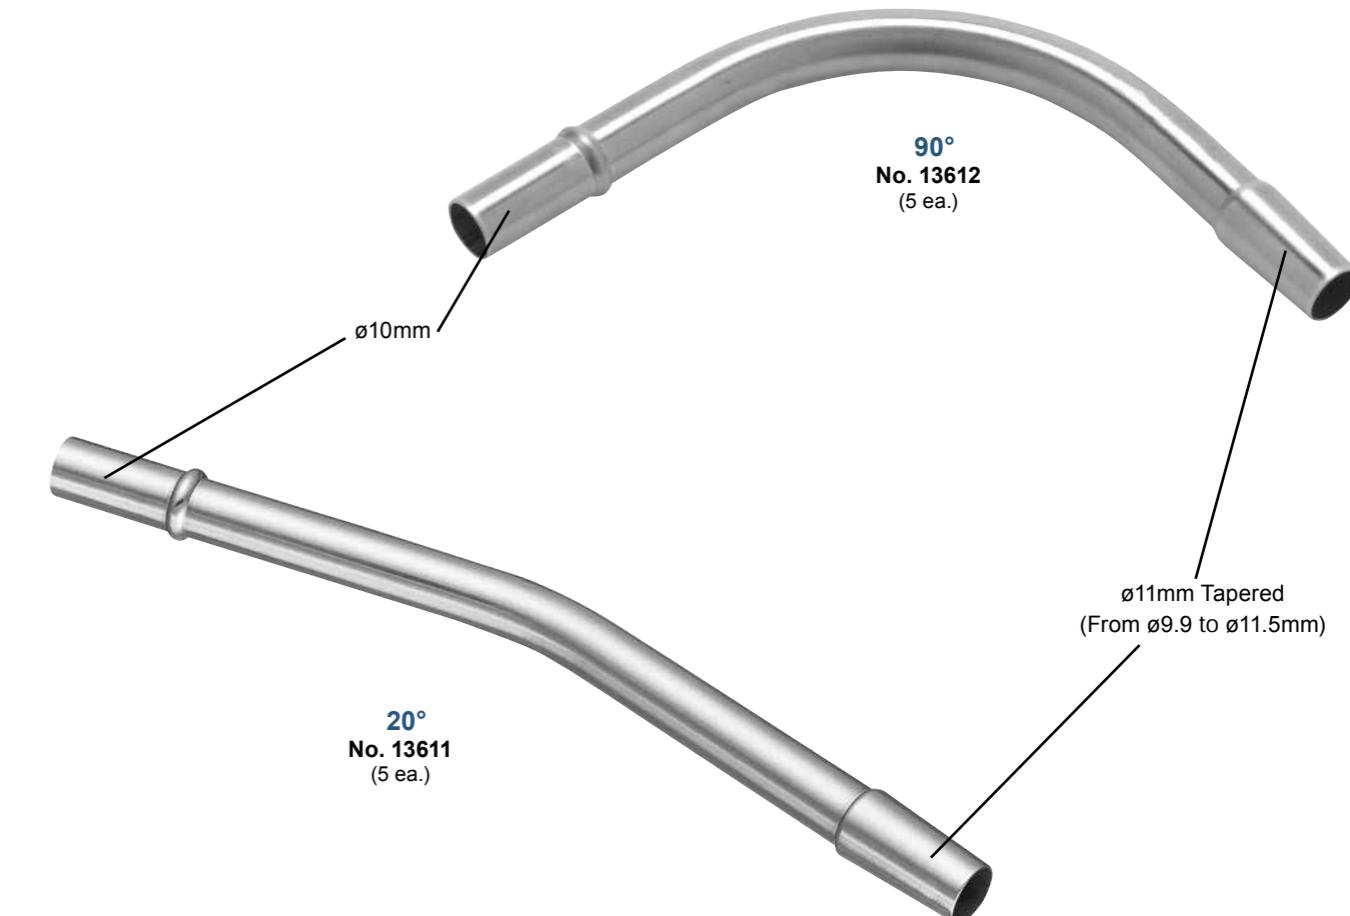

## Temporary Filling Carrier

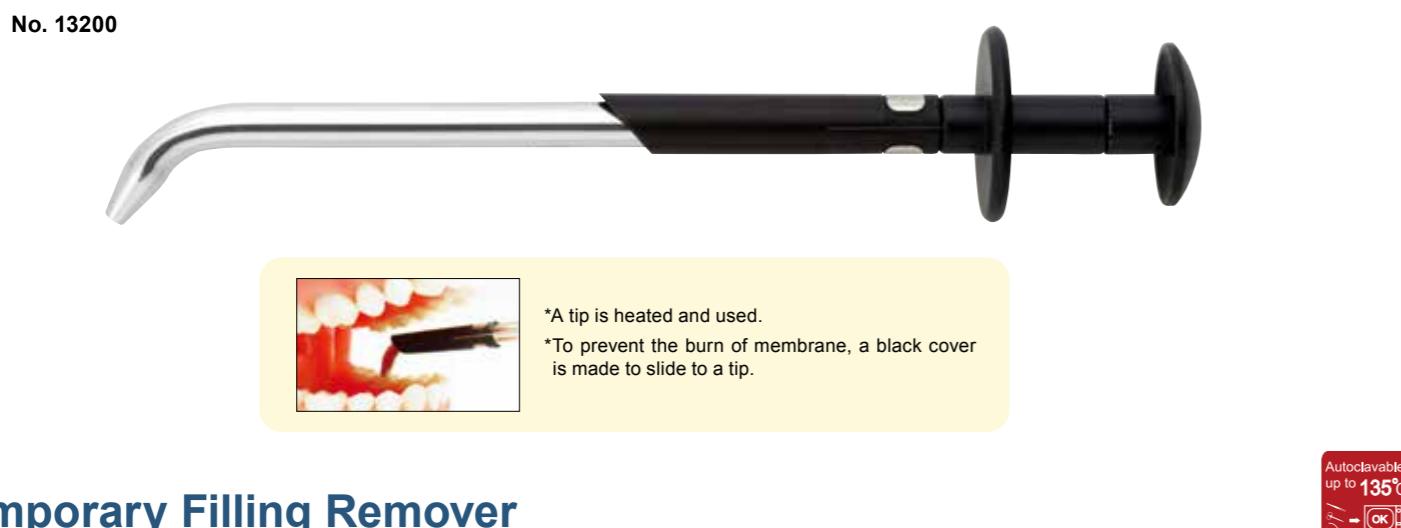

## Temporary Filling Remover



## Sold Separately

## Rubber Sleeve

No. 13613  
(5 ea.)

Autoclavable up to 135°C  
Avoid Ultraviolet Sterilization



\*Size / 40mm  
\*Material / Si

\*\*"Rubber Sleeve" has a trap inside.

## Adapter

No. 13614

Autoclavable up to 135°C  
Avoid Ultraviolet Sterilization



\*In case the inside diameter of evacuation tube is 16mm, this adaptor is needed for the use of "Evacuation Tip Universal".

\*Material / PTFE

## Cleaning Brush L (ø12mm)

No. 13653  
(12 ea.)

Not Autoclavable



Size / 180mm



## Stainless Dish

\*Excellent when using small portion of bath such as topical anesthesia, local disinfection, etching solution, and temporary filling material (powder or liquid).



No. 13670  
(5 ea.)



\*Hole diameter / ø16mm  
\*Size / W56 x D31 x H8.5mm

## Stainless Tray



M  
No. 13413



Size / W245 x D146 x H8mm



S  
No. 13410

Size / W245 x D73 x H8mm

